

# Qualitative ELISA for Bt-Cry1Ab/1Ac

Cat. No: KBA001D

Immunoassay for qualitative screening of Cry1Ab and Cry1Ac proteins in transgenic crops

For use in assessment of transgenic proteins in Agriculture Only. Not for use in Human or Animal diagnostic or therapeutic procedures. Purchase does not include or carry the right to resell or transfer this product either as a stand-alone product or as a component of another product. Any use of this product other than the permitted use without the express written authorization of KRISHGEN BioSystems is strictly prohibited.

**KRISHGEN BioSystems** 135/37, Sonawala Bldg, 2<sup>nd</sup> Floor, Zaveri Bazar, Mumbai 400 002  
Tel: 91-22-66372990/91 Fax: 91-22-66372991 E-mail: [sales@krishgen.com](mailto:sales@krishgen.com) Website: [www.krishgen.com](http://www.krishgen.com)

**Introduction:**

*B. thuringiensis* forms crystals of proteinaceous insecticidal  $\delta$ -endotoxins (Cry toxins) which are encoded by **cry** genes. Many genetically engineered crops have been developed with insect tolerance till date by expressing cry genes from *Bacillus thuringiensis*. Bt-modified crops appear to be safe for farmers and consumers.

**Intended Use:**

Bt-Cry1Ab/Ac ELISA assay is used for qualitative laboratory screening of both Bt-Cry1Ab and Bt-Cry1Ac proteins in leaves, seedlings and seeds of transgenic crop varieties like cotton and corn. The assay cannot be used to distinguish between Bt-Cry1Ab and Bt-Cry1Ac proteins.

**Principle:**

The Bt-Cry1Ab/1Ac Qualitative kit is an Enzyme-Linked Immunosorbent Assay (ELISA).

Plant leaf or seed sample extracts are added to microtiter plate, which is coated with antibodies to Cry1Ab/Cry1Ac toxin. If Bt-Cry1Ab protein or Bt-Cry1Ac protein is present in the sample, it binds to the antibody and thus is captured in the wells, which can then be detected by addition of an enzyme Conjugate. This immunological reaction results in formation of a sandwich complex of solid phase antibody-toxin-enzyme labeled antibody. The wells are washed to remove any unbound reactants as per the wash procedure (see Assay procedure section mentioned below). The substrate is then reacted. If any enzyme is present the substrate will be hydrolysed signifying the presence of Bt-Cry1Ab or Bt-Cry1Ac protein. This color reaction can be measured spectrophotometrically or observed visually. The color development is proportional to the concentration of Cry1Ab/Cry1Ac toxin in the sample extract.

**Materials Provided:**

1. Microtitre coated plate (96 wells) – 1 no
2. Enzyme Conjugate, 6 ml – 1 bottle
3. Positive Control – 1 vial
4. Substrate, 11ml – 1 bottle
5. Wash Buffer (20X) – 10 mL
6. Extraction Buffer (20X) – 3 mL
7. Stop Solution, 11 ml – 1 bottle
8. Instruction Manual

**Materials to be provided by the End-User:**

1. Grinding equipment
2. Microplate Reader able to measure absorbance at 450 nm.
3. Adjustable pipettes to measure volumes ranging from 50  $\mu$ l to 25 ml.
4. Deionized (DI) water.
5. Wash bottle or automated microplate washer.
7. Timer.
8. Absorbent paper.

**Handling/Storage:**

1. Reconstitute or dilute only the specific reagents mentioned in the reagent preparation section, when ready to run the assay.
2. Store all kit components at 4<sup>o</sup>C to 8<sup>o</sup>C when not in use and do not expose them to temperatures greater than 37<sup>o</sup>C or less than 2<sup>o</sup>C
3. Do not use kit components after the expiration date.
4. Do not repeatedly freeze/thaw the reagents as loss of activity may result.
5. Before using, bring all components to room temperature (18-25 °C). Upon assay completion return all components to appropriate storage conditions.
6. ELISA plate pouches contain dessicant. Keep the plates sealed in the pouch with dessicant in the refrigerator when not in use.

**Health Hazard Warnings:**

1. Reagents that contain preservatives may be harmful if ingested, inhaled or absorbed through the skin.
2. Handle Stop Solution carefully. Obtain medical attention in case of accidental ingestion of kit components.
3. Avoid assay of samples containing Sodium azide as it is hazardous.

**Reagent Preparation (all reagents should be diluted immediately prior to use):**

1. Dilute the 20X Extraction buffer to 60 mL to make 1X concentrate
2. Prepare a sufficient amount of wash solution (1X) by diluting the 20X Wash Buffer (10 mL) to 190 mL of de-ionized or distilled water. Crystallization of the undiluted wash buffer may occur and can be dissolved by warming.

**Sample preparation:**

The extraction protocols need to be validated by the individual users. Prevent sample-to-sample cross contamination.

*Recommended Protocol –*

- **Leaf samples** – Take green, actively growing leaf samples. Punch 2 to 3 leaf disc samples with the eppendorf in which the extraction is to be carried out and extract it by adding 0.5 to 1 ml extraction buffer. Allow the solids to settle and use the extract for the assay
- **Seed sample** – crush or grind the seed sample into powder and extract it with 0.5 to 1 ml of extraction buffer. Allow the solids to settle and use the extract for the assay


**Procedural Notes:**

1. Read all the instructions thoroughly before performing the test.
2. Allow all reagents to reach room temperature before beginning and reconstitute or dilute the required reagents.
3. In order to achieve good assay reproducibility and sensitivity, proper washing of the plates to remove excess unreacted reagents is essential.

4. All standards, controls and samples should be assayed atleast in duplicates.
5. If the substrate has a distinct blue color prior to use it may have been contaminated and use of such substrate can lead to compromisation of the sensitivity of the assay.
6. The assay has been optimized to be used with the protocol mentioned. Any deviation from the same may invalidate the results.

**Assay Procedure:**

1. Bring all reagents to room temperature prior to use. It is strongly recommended that all standards and samples be run in duplicates or triplicates.
2. Add 50  $\mu$ L of **Extraction buffer** as Blank, 50  $\mu$ L of **Positive Control** and 50  $\mu$ L of **Sample extract** to respective wells. Cover the microplate with a parafilm.
3. Mix the contents in the wells by moving the plate in rapid circular motion, see to it that the contents do not spill.
4. Incubate at room temperature for 30 minutes or alternatively place on an orbital shaker at about 200rpm for 20 minutes.
5. Add 50  $\mu$ L of **Enzyme Conjugate** to each well and cover the plate with a parafilm and incubate it at room temperature for 1 hour or use an orbital shaker at 200 rpm for 45 minutes.
6. Aspirate and wash plate 4 times with **Wash Buffer** and blot residual buffer by firmly tapping plate upside down on absorbent paper. Wipe of any liquid from the bottom outside of the microtiter wells as any residue can interfere in the reading step. All the washes should be performed similarly or alternatively a microtiter plate / strip washer may be used.
7. Add 100  $\mu$ L of **Substrate** solution into each well of the plate. Cover the plate with a parafilm and incubate for 30 minutes at ambient temperature or place on an orbital shaker at 200rpm.
8. Add 100  $\mu$ L of **Stop Solution** to each well. This will turn the well contents yellow.
9. Measure the optical density of the wells on a plate reader at 450 nm within 30 minutes.

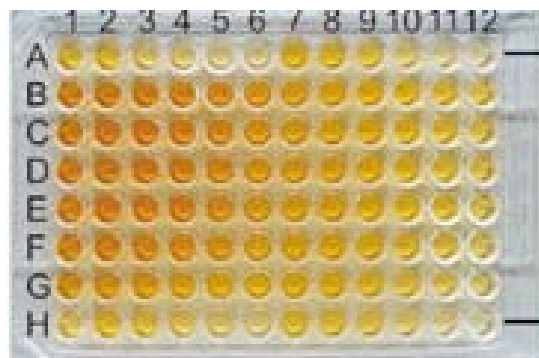

**Interpretation of the Results:**

Compare the OD's of sample extracts with Positive controls and blank wells. Those with absorbance close to blank well are said to be negative i.e. free of Cry1Ab/1Ac toxin, whereas those with absorbance close to positive control or significantly higher than blank well are considered positive i.e. transgenic.

**Precautions:**

1. Do not mix reagents from different kits or lots. Reagents and/or antibodies from different manufacturers should not be used with this set.
2. Substrate is light and heat sensitive hence do not expose it to direct sunlight while pipetting or incubating. Cry1Ab/Ac proteins can also be degraded by heat and sunlight.
3. Samples and kit reagents after use should be disposed off observing appropriate regulations.
4. If necessary it is recommended that the results should be confirmed by an alternative method.
5. Do not dilute or adulterate test reagents or use samples not called for in the test procedure.

**Quality Control:**

It is recommended that for each laboratory assay, appropriate quality control samples in each run to be used to ensure that all reagents and procedures are correct.

**A typical assay setup**

	1	2	3	4	5	6	7	8	9	10	11	12
<b>A</b>	Blank	S4	S8	S12	S16	S20	S24	S28	S32	S36	S40	S44
<b>B</b>	P.C	S4	S8	S12	S16	S20	S24	S28	S32	S36	S40	S44
<b>C</b>	S1	S5	S9	S13	S17	S21	S25	S29	S33	S37	S41	S45
<b>D</b>	S1	S5	S9	S13	S17	S21	S25	S29	S33	S37	S41	S45
<b>E</b>	S2	S6	S10	S14	S18	S22	S26	S30	S34	S38	S42	S46
<b>F</b>	S2	S6	S10	S14	S18	S22	S26	S30	S34	S38	S42	S46
<b>G</b>	S3	S7	S11	S15	S19	S23	S27	S31	S35	S39	S43	P.C
<b>H</b>	S3	S7	S11	S15	S19	S23	S27	S31	S35	S39	S43	Blank

\* All controls and samples are run in duplicates

Blank – Blank wells  
 P.C – Positive control wells  
 S. – Sample extract wells

**THANK YOU FOR USING KRISHGEN PRODUCT !**

**LIMITED WARRANTY**

Krishgen Biosystems does not warrant against damages or defects arising in shipping or handling, or out of accident or improper or abnormal use of the Products; against defects in products or components not manufactured by Krishgen Biosystems, or against damages resulting from such non-Krishgen Biosystems made products or components. Krishgen Biosystems passes on to customer the warranty it received (if any) from the maker thereof of such non Krishgen made products or components. This warranty also does not apply to Products to which changes or modifications have been made or attempted by persons other than pursuant to written authorization by Krishgen Biosystems.

THIS WARRANTY IS EXCLUSIVE. The sole and exclusive obligation of Krishgen Biosystems shall be to repair or replace the defective Products in the manner and for the period provided above. Krishgen shall not have any other obligation with respect to the Products or any part thereof, whether based on contract, tort, strict liability or otherwise. Under no circumstances, whether based on this Limited Warranty or otherwise, shall Krishgen Biosystems be liable for incidental, special, or consequential damages.

This Limited Warranty states the entire obligation of Krishgen Biosystems with respect to the Products. If any part of this Limited Warranty is determined to be void or illegal, the remainder shall remain in full force and effect.

*Parafilm is a registered trademark of American Can Corporation  
Bollgard and Bollgard II are registered trademarks of Monsanto Technology LLC  
WideStrike is a trademark of Dow AgroSciences LLC  
Krishgen Biosystems. 2009*