

KRIBIOLISA™ Buserelin (Suprefact) ELISA

REF : KBI5003

Ver 2.0

RUO

Immunoassay for Quantitative estimation of Buserelin in human serum and plasma.

RUO	For Research Use Only	REF	Catalog Number
	Store At	LOT	Batch Code
	Manufactured By		Biological Risk
	Expiry Date		Consult Operating Instructions

For Research Use Only. Purchase does not include or carry the right to resell or transfer this product either as a stand-alone product or as a component of another product. Any use of this product other than the permitted use without the express written authorization of KRISHGEN BioSystems is strictly prohibited.

REF KBI5003

96 tests



KRISHGEN BioSystems | For US / Europe: toll free +1(888)-970-0827 tel: +1(562)-568-5005

For Asia / India: tel: +91(22)-49198700

Email: sales1@krishgen.com

Introduction:

Buserelin is a LHRH agonist used for the palliative treatment of hormone-dependent advanced carcinoma of the prostate gland in males and treatment of endometriosis in females. Buserelin may be used in the treatment of hormone-responsive cancers such as prostate cancer or breast cancer, estrogen-dependent conditions (such as endometriosis or uterine fibroids), and in assisted reproduction. Buserelin stimulates the pituitary glands gonadotropin-releasing hormone receptor (GnRHR). Buserelin desensitizes the GnRH receptor, reducing the amount of gonadotropin. In males, this results in a reduction in the synthesis and release of testosterone. In females, estrogen secretion is inhibited. While initially, there is a rise in FSH and LH levels, chronic administration of Buserelin results in a sustained suppression of these hormones.

Intended Use:

The KRIBIOLISA™ Buserelin (Suprefact) ELISA kit is used for estimation of Buserelin in solutions and human serum.

Principle:

The Buserelin ELISA is a competitive immunoassay for the determination of Buserelin. The GnRH antibodies are coated on 96 well plate. A constant concentration of Buserelin HRP:Conjugate and varying concentration of unlabeled Buserelin or sample compete for binding to the capture antibody. Buserelin HRP: Conjugate which produces a soluble colored product after addition of TMB substrate. The enzyme reaction is stopped by dispensing of stop solution into the wells. The optical density (OD) of the solution at 450 nm is inversely proportional to the amount of bound Buserelin present in standards or samples.

Materials Provided:

Part	Description	Qty
Coated Microtiter Plate	96 well polystyrene microplate (12 strips of 8 wells) coated with GnRH antibody.	1 x 96 wells
Buserelin Standard	Recombinant Buserelin standard (Concentered, 1mg/ml)	20ul
Buserelin HRP : Conjugation	Buserelin conjugated to HRP prepared in buffer with protein stabilizer and preservatives 0.02% methylisothiazolone and 0.02% bromonitrodiroxane	12 ml
(1X) Standard Diluent	Buffered protein base with protein stabilizer and 1:10 human serum and preservative sodium azide < 0.1%	10ml
(1X) Sample Diluent	Buffered protein base with BSA and preservative sodium azide < 0.1%	50ml
(20X) Wash Buffer	20-fold concentrated solution of buffered surfactant with preservative thiomersol < 0.01%. May turn yellow over time.	25 ml
TMB Substrate	Stabilized Chromogen	12 ml
Stop Solution	0.73M Phosphoric Acid	12 ml
Instruction Manual		1 no

Materials to be provided by the End-User:

1. Microplate Reader able to measure absorbance at 450 nm.
2. Adjustable pipettes to measure volumes ranging from 50 ul to 1000 ul.
3. Deionized (DI) water.
4. Wash bottle or automated microplate washer.
5. Graph paper or software for data analysis.
6. Tubes to prepare standard/sample dilutions.
7. Timer.
8. Absorbent paper.
9. Incubator.

Storage Information:

1. Store kit components at 2-8°C.
2. All the reagents and wash solutions should be used within 12 months from manufacturing date. Before using, bring all components to room temperature (18-25°C).
3. Before using, bring all components to room temperature (18-25°C). Upon assay completion return all components to appropriate storage conditions

Health Hazard Warnings:

1. Reagents that contain preservatives may be harmful if ingested, inhaled or absorbed through the skin. Refer to the MSDS online for details.

Specimen Collection and Handling:

Blood is taken by venipuncture. Serum is separated after clotting by centrifugation. Plasma can be used too. Lipaemic, hemolytic or contaminated samples should not be run. Repeated freezing and thawing should be avoided. If samples are to be used for several assays, initially aliquot samples and keep at -20°C.

For Serum & Plasma - Samples have to be **diluted 1:10 (v/v)**, e.g. **10 ul sample + 90 ul Sample Diluent** prior to assay. The samples may be kept at 2 - 8°C for up to three days. Long-term storage requires -20°C.

Reagent Preparation (all reagents should be diluted immediately prior to use):

1. Bring all kit components and samples to room temperature (18-25°C) before use. If the kit will not be used up in one time, please only take out strips and reagents for present experiment, and leave the remaining strips and reagents in required condition.
2. To make **Wash Buffer (1X)**; dilute 25 ml of 20X Wash Buffer in 475 ml of DI water.
3. **Standard:** Original standard provide in kit is 1 mg/ml. Add 1 ul of standard to 999 ul of Standard Diluent to give 1ug/ml middle stock. Use this middle stock to prepare the remaining standards as per the below table. Standard Diluent (1X) serves as the zero standard (0 ng/ml).

Standard Concentration	Standard No	Dilution Particulars
1 ug/ml	Middle stock	1ul of original standard + 999 ul Standard Diluent (1X)
75 ng/ml	Standard No.6	18.75ul of Middle stock + 231.25 ul of Standard Diluent (1X)
37.5 ng/ml	Standard No.5	125 ul of Standard No. 6 + 125 ul Standard Diluent (1X)
18.75 ng/ml	Standard No.4	125 ul of Standard No. 5 + 125 ul Standard Diluent (1X)
9.375 ng/ml	Standard No.3	125 ul of Standard No. 4 + 125 ul Standard Diluent (1X)
4.668 ng/ml	Standard No.2	125 ul of Standard No. 3 + 125 ul Standard Diluent (1X)
2.344 ng/ml	Standard No.1	125 ul of Standard No. 2 + 125 ul Standard Diluent (1X)
0 ng/ml	Standard No.0	Only Standard Diluent (1X)

Procedural Notes:

1. In order to achieve good assay reproducibility and sensitivity, proper washing of the plates to remove excess un-reacted reagents is essential.
2. Avoid assay of Samples containing Sodium Azide (NaN₃), as it could destroy the HRP activity resulting in under-estimation of the amount of Buserelin.
3. It is recommended that all Standards and Samples be assayed in duplicates.
4. Maintain a repetitive timing sequence from well to well for all the steps to ensure that the incubation timings are same for each well.
5. If the Substrate has a distinct blue color prior to use it may have been contaminated and use of such substrate can lead to low / incorrect results.

6. The plates should be read within 30 minutes after adding the Stop Solution.
7. It is advisable to make a work list in order to identify the location of Standards and Samples.

Assay Procedure:

1. It is strongly recommended that all Standards and Samples be run in duplicates or triplicates. A standard curve is required for each assay. All steps must be performed at RT.
2. Pipette **100 ul** of prepared **Standards** or diluted **Samples** into the respective wells.
3. Pipette **100 ul** of **Buserelin HRP : Conjugate** into each well
4. Cover the plate and incubate for 150 minutes at 37°C.
5. Add **100 ul** of **TMB Substrate** in each well.
6. Incubate the plate at 37°C for 30 minutes in dark. DO NOT SHAKE or else it may result in higher backgrounds and worse precision. Positive wells should turn bluish in color.
7. Pipette out **100 ul** of **Stop Solution**. Wells should turn from blue to yellow in color.
8. Read the absorbance at 450 nm with a microplate reader.

Calculation of Results:

Determine the Mean Absorbance for each set of duplicate Standards and Samples. Using Graph paper, plot the average value (absorbance 450nm) of each standard on the Y-axis versus the corresponding concentration of the standards on the X-axis. Draw the best fit curve through the standard points. To determine the unknown Buserelin concentrations, find the unknown's Mean Absorbance value on the Y-axis and draw a horizontal line to the standard curve. At the point of intersection, draw a vertical line to the X-axis and read the Buserelin concentration. If samples were diluted, multiply by the appropriate dilution factor.

Software which is able to generate a linear regression like cubic spline or 4PL (2nd order) is best recommended for automated results.

Note:


It is recommended to repeat the assay at a different dilution factor in the following cases:

- If the sample absorbance value is below the first standard.
- If the absorbance value is equivalent or higher than the 75 ng/ml standard.

Typical Data

Standard Concentration (ng/ml)	Mean Absorbance	Interpolated Concentration	% Interpolated Concentration against Actual Concentration
0	2.121		--
2.344	1.565	2.3	96.1
4.688	1.345	4.7	99.3
9.375	1.052	11.0	117.6
18.75	0.952	14.8	78.8
37.50	0.618	44.1	117.6
75	0.499	72.1	96.1

Typical Graph

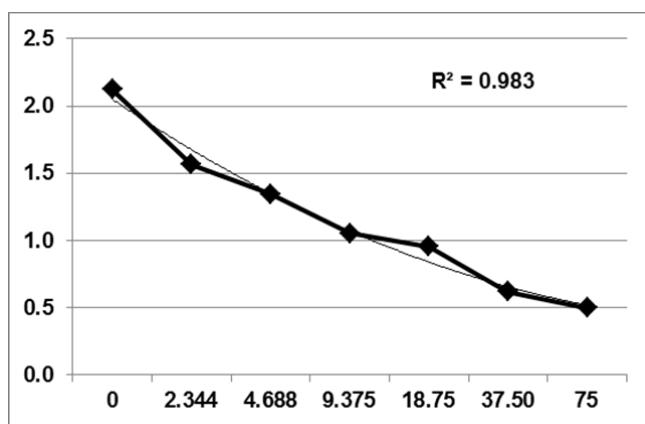

Quality Control:

It is recommended that for each laboratory assay appropriate quality control samples in each run to be used to ensure that all reagents and procedures are correct.

Performance Characteristics of the Kit:

This kit has been validated as per EMA/FDA guidelines in line with ICH Code for Harmonization of Biological Assays.

Sensitivity:

Limit Of Detection: It is defined as the lowest detectable concentration corresponding to a signal of Mean of '0' standard plus 2* SD.

10 replicates of '0' standards were evaluated and the LOD was found to be ~2.2 ng/ml

Specificity:

The calibrators used are certified against commercially available Suprefact™.

Linearity:

Standards provided in the kit will be used for measuring the linearity range of Buserelin present in matrix. The standard graph range indicated is 0 ng/ml to 75 ng/ml.

Precision:

Precision is defined as the percent coefficient of variation (%CV) i.e. standard deviation divided by the mean and multiplied by 100. Assay precision was determined by both intra (n=5 assays) and inter assay (n=5 assays) reproducibility on two pools with low (2.3ng/ml), medium (18.75ng/ml) and high (75ng/ml) concentrations. While actual precision may vary from laboratory to laboratory and technician to technician, it is recommended that all operators achieve precision below these design goals before reporting results.

Pool	Intra Assay %CV	Inter Assay %CV
Low	<10%	<10%
Medium	<5%	<5%
High	<5%	<5%


Safety Precautions:

- **This kit is For Research Use Only.** Follow the working instructions carefully.
- The expiration dates stated on the kit are to be observed. The same relates to the stability stated for reagents
- Do not use or mix reagents from different lots.
- Do not use reagents from other manufacturers.
- Avoid time shift during pipetting of reagents.
- All reagents should be kept in the original shipping container.
- Some of the reagents contain small amount of sodium azide (< 0.1 % w/w) as preservative. They must not be swallowed or allowed to come into contact with skin or mucosa.
- Source materials maybe derived from human body fluids or organs used in the preparation of this kit were tested and found negative for HBsAg and HIV as well as for HCV antibodies. However, no known test guarantees the absence of such viral agents. Therefore, handle all components and all patient samples as if potentially hazardous.
- Since the kit contains potentially hazardous materials, the following precautions should be observed
 - Do not smoke, eat or drink while handling kit material
 - Always use protective gloves
 - Never pipette material by mouth
 - Wipe up spills promptly, washing the affected surface thoroughly with a decontaminant.
- In any case GLP should be applied with all general and individual regulations to the use of this kit.




SCHEMATIC ASSAY PROCEDURE

1. Remove all components, 30 minutes before adding into the assay plate.

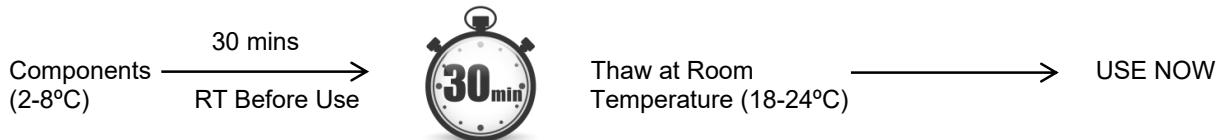

2. Avoid repeated cool-thaw of the components as there will be a loss of activity and this can affect the results.

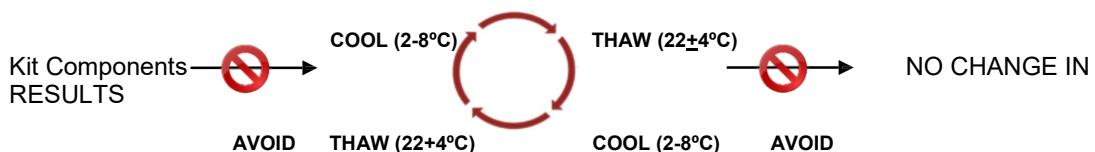


3. Pipette **100 ul prepared Standards / diluted Samples** into each well.



4. Pipette **100 ul Buserelin HRP:Conjugation** into the respective wells.




5. Cover plate and incubate for **150 min** at 37°C.




6. Aspirate and wash wells 4 times with **Wash Buffer (1X)**.



7. Pipette **100 ul TMB Substrate** into each well.



8. Cover plate and incubate for **30 min** at 37°C.



9. Pipette **100 ul Stop Solution** into each well.



10. Read absorbance at 450nm with a microplate reader within **30 min** of stopping reaction.



Typical Example of a Work List

Well #	Contents	Absorbance at 450nm	Mean Absorbance	ng/ml Buserelin equivalent
1A	0 ng/ml			
2A	0 ng/ml			
1B	2.344 ng/ml			
2B	2.344 ng/ml			
1C	4.688 ng/ml			
2C	4.688 ng/ml			
1D	9.375 ng/ml			
2D	9.375 ng/ml			
1E	18.75 ng/ml			
2E	18.75 ng/ml			
1F	37.5 ng/ml			
2F	37.5 ng/ml			
1G	75 ng/ml			
2G	75 ng/ml			
1H	Sample			
2H	Sample			
3A	Sample			
4A	Sample			

LIMITED WARRANTY

Krishgen Biosystems does not warrant against damages or defects arising in shipping or handling, or out of accident or improper or abnormal use of the Products; against defects in products or components not manufactured by Krishgen Biosystems, or against damages resulting from such non-Krishgen Biosystems made products or components. Krishgen Biosystems passes on to customer the warranty it received (if any) from the maker thereof of such non Krishgen made products or components. This warranty also does not apply to Products to which changes or modifications have been made or attempted by persons other than pursuant to written authorization by Krishgen Biosystems.

THIS WARRANTY IS EXCLUSIVE. The sole and exclusive obligation of Krishgen Biosystems shall be to repair or replace the defective Products in the manner and for the period provided above. Krishgen Biosystems shall not have any other obligation with respect to the Products or any part thereof, whether based on contract, tort, and strict liability or otherwise. Under no circumstances, whether based on this Limited Warranty or otherwise, shall Krishgen Biosystems be liable for incidental, special, or consequential damages.

This Limited Warranty states the entire obligation of Krishgen Biosystems with respect to the Products. If any part of this Limited Warranty is determined to be void or illegal, the remainder shall remain in full force and effect.

Krishgen Biosystems. 2024

THANK YOU FOR USING KRISHGEN PRODUCT!

KRISHGEN BIOSYSTEMS®, GENLISA®, DHARMAPLEX™, GENBULK™, GENLISA™, KRISHZYME®, KRISHGEN®, KRIBIOLISA®, KRISHPLEX®, TITANIUM®, QUALICHEK® are registered trademarks of KRISHGEN BIOSYSTEMS. ©KRISHGEN BIOSYSTEMS. ALL RIGHTS RESERVED.

KRISHGEN BIOSYSTEMS | OUR REAGENTS | YOUR RESEARCH |

SYMBOLS KEY

	Coated Microtiter Plate (12x8 wells)
	Buserelin Standard
	Buserelin HRP:Conjugation
	(1X) Standard Diluent
	(1X) Sample Diluent
	(20X) Wash Buffer
	TMB Substrate
	Stop Solution
	Consult Instructions for Use
	Catalog Number
	Expiration Date
	Storage Temperature