






GENLISA™ Human SARS-CoV-2 (Covid-19) Nucleocapsid Omicron Variant (B.1.1.529) Antigen Quantitative TITRATION ELISA

REF : KBVH015-47

Ver 1.0


RUO

Enzyme Immunoassay for the Quantitative Antigen Determination of SARS-CoV-2 (Covid-19) Omicron Variant (B.1.1.529) in human serum and plasma and cell culture supernatant

RUO	For Research Use Only	REF	Catalog Number
	Store At	LOT	Batch Code
	Manufactured By		Biological Risk
	Expiry Date		Consult Operating Instructions

For Research Use Only. Purchase does not include or carry the right to resell or transfer this product either as a stand-alone product or as a component of another product. Any use of this product other than the permitted use without the express written authorization of KRISHGEN BioSystems is strictly prohibited.

REF KBVH015-47

 96 tests

KRISHGEN BioSystems For US/Europe Customers: toll free +1(888)-970-0827 | tel +1(562)-568-5005
 For Asia/India Customers: tel +91(22)-49198700
 Email: sales@krishgen.com | http://www.krishgen.com

Introduction:

The GENLISA™ ELISA kits are used for assessing the specific biomarker in samples analytes which may be serum, plasma and cell culture supernatant as validated with the kit. The kit employs a sandwich ELISA technique which leads to a higher specificity and increased sensitivity compared to conventional competitive ELISA kits which employ only one antibody. Double antibodies are used in this kit.

Intended Use:

The GENLISA™ Human SARS-CoV-2 (Covid-19) Nucleocapsid Omicron Variant (B.1.1.529) Antigen Quantitative TITRATION ELISA kit is used as an analytical tool for quantitative antigen determination of Human SARS-CoV-2 (Covid-19) Nucleocapsid Omicron Variant (B.1.1.529) in human serum and plasma and cell culture supernatant.

Principle:

The method employs sandwich ELISA technique. Monoclonal antibodies are pre-coated onto microwells. Samples and standards are pipetted into microwells and Human SARS-CoV-2 (Covid-19) Nucleocapsid Omicron Variant (B.1.1.529) present in the sample are bound by the capture antibodies. After incubation the wells are washed and followed by HRP- conjugated Detection Antibody is pipetted and incubated to form a complex. After washing microwells in order to remove any non-specific binding, the substrate solution (TMB) is added to microwells and color develops proportionally to the amount of Human SARS-CoV-2 (Covid-19) Nucleocapsid Omicron Variant (B.1.1.529) in the sample. Color development is then stopped by addition of stop solution. Absorbance is measured at 450 nm.

Materials Provided:

Part	Description	Qty
SARS-CoV-2 (Covid-19) spike Nucleocapsid Omicron Variant (B.1.1.529) protein Antibody Coated Microtiter Plate	96 well polystyrene microplate (12 strips of 8 wells) coated with SARS-CoV-2 (Covid-19) Nucleocapsid Omicron Variant (B.1.1.529) Antibody	1 x 96 wells
Human SARS-CoV-2 Nucleocapsid Omicron Variant (B.1.1.529) protein Standard	Lyophilized Human SARS-CoV-2 Nucleocapsid Omicron Variant (B.1.1.529) protein Standard Concentration – 5 ug/ml	2 vials
SARS-CoV-2 (Covid-19) Antibody:HRP Conjugate	SARS-CoV-2 (Covid-19) Nucleocapsid Omicron Variant (B.1.1.529) Antibody:HRP Conjugate prepared in buffer with protein stabilizer and preservatives 0.02% methylisothiazolone and 0.02% bromonitrodioxane.	12 ml
(5X) Sample Diluent	Buffered protein base with preservative thiomersol < 0.01%	50 ml
(1X) Standard Diluent	Buffered protein base with preservative thiomersol < 0.01% with 1:100 dilution human serum	10 ml
(20X) Wash Buffer	20-fold concentrated solution of buffered surfactant with preservative thiomersol < 0.01%. May turn yellow over time.	25 ml
TMB Substrate	Stabilized Chromogen	12 ml
Stop Solution	2N Sulfuric Acid	12 ml
Instruction Manual		1 no

Materials to be provided by the End-User:

1. Microtiter Plate Reader able to measure absorbance at 450 nm.
2. Adjustable pipettes and multichannel pipettor to measure volumes ranging from 25 ul to 1000 ul
3. Deionized (DI) water
4. Wash bottle or automated microplate washer
5. Graph paper or software for data analysis
6. Timer
7. Absorbent Paper

Handling/Storage:

1. Store main kit components at 2-8°C.
2. Before using, bring all components to room temperature (18-25°C). Upon assay completion return all components to appropriate storage conditions.
3. The Substrate is light-sensitive and should be protected from direct sunlight or UV sources.

Health Hazard Warnings:

1. Reagents that contain preservatives may be harmful if ingested, inhaled or absorbed through the skin.



Sample Preparation and Storage:

Specimens should be clear and non-hemolyzed. Samples should be run at a number of dilutions to ensure accurate quantitation.

Blood is taken by venipuncture. Serum is separated after clotting by centrifugation. Plasma can be used, too. Lipaemic, hemolytic or contaminated samples should not be run. Repeated freezing and thawing should be avoided.

Samples should be diluted 1:100 (v/v) for optimal recovery, (for example 1 ul sample + 99 ul (1X) Sample Diluent) prior to assay. In cases where matrix interferences is under or over observed, the samples may be diluted with (1X) Sample Diluent accordingly.

The samples may be kept at 2 - 8°C for up to three days. For long-term storage please store at -20°C.

Note: Grossly hemolyzed samples are not suitable for use in this assay

Cell Culture Supernates - Remove particulates by centrifugation and assay immediately or aliquot and store samples at -20°C or lower temperature. Avoid repeated freeze-thaw cycles. If the use of original supernate sample or low dilution (<5 fold) are necessary due to the expected low concentration of antigen supernates need be adjust to neutral pH condition before assay.

Note:

The sample should be diluted to within the working range of the assay in 1X Sample Diluent. The exact dilution must be determined based on the concentration of specific target in individual samples.

Reagent Preparation (all reagents should be diluted immediately prior to use):

1. Label any aliquots made with the kit Lot No and Expiration date and store it at appropriate conditions mentioned.
2. Bring all reagents to Room Temperature before use.
3. To make **Sample Diluent (1X)**; dilute **50 ml** of **5X Sample Diluent** in **200 ml of DI water**.
4. To make **Wash Buffer (1X)**; dilute **25 ml** of **20X Wash Buffer** in **475 ml of DI water**.
5. **Standards Preparation:** Reconstitute the concentrated Standard lyophilized vial with 1 ml of Standard Diluent (1X) to obtain a concentration of 5ug/ml. Keep the vial for 15 mins with gentle agitation before making further dilutions. Dilute 400 ul of original **Standard (5 ug/ml)** with 100 ul of Standard Diluent (1X) to generate a **4000 ng/ml Standard Solution**. Prepare further **Standards** by serially diluting the Standard Solution as per the below table. Use the Standard Diluent (1X) as the Zero Standard (Standard No.0).

Standard Concentration	Standard Vial	Dilution Particulars
5 ug/ml	Original Standard	Original Standard provided in the Kit + 1ml Standard Diluent (1X)
4000 ng/ml	Standard No.7	400 ul Original Standard (5 ug/ml) + 100 ul Standard Diluent (1X)
2000 ng/ml	Standard No.6	250 ul Standard No.7 + 250 ul Standard Diluent (1X)
1000 ng/ml	Standard No.5	250 ul Standard No.6 + 250 ul Standard Diluent (1X)
500 ng/ml	Standard No.4	250 ul Standard No.5 + 250 ul Standard Diluent (1X)
250 ng/ml	Standard No.3	250 ul Standard No.4 + 250 ul Standard Diluent (1X)
125 ng/ml	Standard No.2	250 ul Standard No.3 + 250 ul Standard Diluent (1X)

62.5 ng/ml	Standard No.1	250 ul Standard No.2 + 250 ul Standard Diluent (1X)
0 ng/ml	Standard No. 0	Only Standard Diluent (1X)

Procedural Notes:

1. In order to achieve good assay reproducibility and sensitivity, proper washing of the plates to remove excess un-reacted reagents is essential.
2. Avoid assay of Samples containing sodium azide (NaN₃), as it could destroy the HRP activity resulting in erroneous results for the presence of Human SARS-CoV-2 (Covid-19).
3. It is recommended that the Standards and Samples be assayed in duplicates.
4. Maintain a repetitive timing sequence from well to well for all the steps to ensure that the incubation timings are same for each well.
5. If the Substrate has a distinct blue color prior to use it may have been contaminated and use of such substrate can lead to compromise of the sensitivity of the assay.
6. The plates should be read within 30 minutes after adding the Stop Solution.
7. Make a work list in order to identify the location of Standards and Samples.

Assay Procedure:

1. Pipette **100 ul** of **Standards** and **diluted Samples** to the respective wells.
2. Seal plate and incubate for 1 hour at 37°C shaking at 180 rpm.
3. Aspirate and wash plate 4 times with **Wash Buffer (1X)** and blot residual buffer by firmly tapping plate upside down on absorbent paper. Wipe of any liquid from the bottom outside of the microtiter wells as any residue can interfere in the reading step. All the washes should be performed similarly.
4. Add **100 ul** of **SARS-CoV-2 Antibody: HRP Conjugate** to each well.
5. Seal plate and incubate for 1 hour at 37°C shaking at 180 rpm.
6. Wash plate 4 times with **Wash Buffer (1X)** as in step 2.
7. Pipette **100 ul** of **TMB Substrate solution**.
8. Incubate in the dark for 30 minutes at Room Temperature.
9. Stop reaction by adding **100 ul** of **Stop Solution** to each well.
10. Read absorbance at 450 nm within 30 minutes of stopping reaction.

Calculation of Results:

Determine the Mean Absorbance for each set of duplicate Standards and Samples. Using Graph Paper, plot the average value (absorbance 450nm) of each standard on the Y-axis versus the corresponding concentration of the standards on the X-axis. Draw the best fit curve through the standard points. To determine the unknown Human SARS-CoV-2 (Covid-19) spike protein concentrations, find the unknown's Mean Absorbance value on the Y-axis and draw a horizontal line to the standard curve. At the point of intersection, draw a vertical line to the X-axis and read the Human SARS-CoV-2 (Covid-19) spike protein Concentration.

If samples were diluted, multiply by the appropriate dilution factor. Software which is able to generate a cubic spline curve-fit or a polynomial 2nd order curve is best recommended for automated results.

Note:

It is recommended to repeat the assay at a different dilution factor in the following cases:
 - If the sample absorbance value is below the first standard.

Quality Control:

It is recommended that for each laboratory assay appropriate quality control samples in each run to be used to ensure that all reagents and procedures are correct.

Safety Precautions:

- **This kit is For Research Use Only.** Follow the working instructions carefully.
- The expiration dates stated on the kit are to be observed. The same relates to the stability stated for reagents
- Do not use or mix reagents from different lots.
- Do not use reagents from other manufacturers.
- Avoid time shift during pipetting of reagents.
- All reagents should be kept in the original shipping container.
- Some of the reagents contain small amount of sodium azide (< 0.1 % w/w) as preservative. They must not be swallowed or allowed to come into contact with skin or mucosa.
- Source materials maybe derived from human body fluids or organs used in the preparation of this kit were tested and found negative for HBsAg and HIV as well as for HCV antibodies. However, no known test guarantees the absence of such viral agents. Therefore, handle all components and all patient samples as if potentially hazardous.
- Since the kit contains potentially hazardous materials, the following precautions should be observed
 - Do not smoke, eat or drink while handling kit material
 - Always use protective gloves
 - Never pipette material by mouth
 - Wipe up spills promptly, washing the affected surface thoroughly with a decontaminant.
- In any case GLP should be applied with all general and individual regulations to the use of this kit.




SCHEMATIC ASSAY PROCEDURE

1. Remove all components, 30 minutes before adding into the assay plate.



2. Avoid repeated cool-thaw of the components as there will be a loss of activity and this can affect the results.

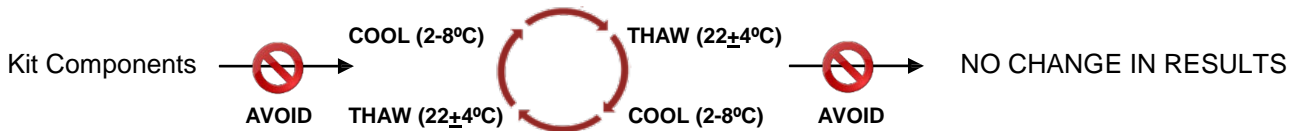

3. Pipette **100 ul Standards** and **diluted Samples** into the respective wells.

4. Cover plate and **incubate** for **60 min** at 37 °C shaking at 180 rpm.

5. Aspirate and wash wells 4 times with **Wash Buffer (1X)**.

6. Pipette **100 ul SARS-CoV-2 Antibody:HRP Conjugate** into each well.

7. Cover plate and **incubate** for **60 min** at 37 °C shaking at 180 rpm.

8. Aspirate and wash wells 4 times with **(1X) Wash Buffer**.

9. Pipette **100 ul TMB Substrate** into each well.

10. Cover plate and **incubate** for **30 min** at Room Temperature.

11. Pipette **100 ul Stop Solution** into each well.

12. Read absorbance at 450nm with a microplate reader within **30 min** of stopping reaction.

Typical Example of a Work List

Well #	Contents	Absorbance at 450nm	Mean Absorbance	Results
1A 2A	0 Standard 0 Standard			
1B 2B	62.5 ng/ml 62.5 ng/ml			
1C 2C	125 ng/ml 125 ng/ml			
1D 2D	250 ng/ml 250 ng/ml			
1E 2E	500 ng/ml 500 ng/ml			
1F 2F	1000 ng/ml 1000 ng/ml			
1G 2G	2000 ng/ml 2000 ng/ml			
1H 2H	4000 ng/ml 4000 ng/ml			
3A 4A	<i>Sample</i>			
3B 4B	<i>Sample</i>			

LIMITED WARRANTY

Krishgen Biosystems does not warrant against damages or defects arising in shipping or handling, or out of accident or improper or abnormal use of the Products; against defects in products or components not manufactured by Krishgen Biosystems, or against damages resulting from such non-Krishgen Biosystems made products or components. Krishgen Biosystems passes on to customer the warranty it received (if any) from the maker thereof of such non Krishgen made products or components.

This warranty also does not apply to Products to which changes or modifications have been made or attempted by persons other than pursuant to written authorization by Krishgen Biosystems.

THIS WARRANTY IS EXCLUSIVE. The sole and exclusive obligation of Krishgen Biosystems shall be to repair or replace the defective Products in the manner and for the period provided above. Krishgen Biosystems shall not have any other obligation with respect to the Products or any part thereof, whether based on contract, tort, and strict liability or otherwise. Under no circumstances, whether based on this Limited Warranty or otherwise, shall Krishgen Biosystems be liable for incidental, special, or consequential damages.

This Limited Warranty states the entire obligation of Krishgen Biosystems with respect to the Products. If any part of this Limited Warranty is determined to be void or illegal, the remainder shall remain in full force and effect.

Krishgen Biosystems. 2022

THANK YOU FOR USING KRISHGEN PRODUCT!